

Bioline™ CHOLERA Ag O1/O139

V. CHOLERAE O1/ O139 ANTIGEN TEST

Bioline™ Cholera Ag O1/O139 test is a rapid immunochromatographic assay for qualitative detection of *Vibrio cholera* O1/O139 in human fecal specimens.


- Easy to use, convenient and clean test
- Specimen : Solid fecal specimen (about 50 mg) or liquid fecal specimen (300 µl)
- Test result : 15 minutes
- Shelf life and storage temperature: 24 months from the date of manufacturing at 1-30 °C
- Performance: Sensitivity 100 %, Specificity 100 % (vs. Culture)



MATERIALS PROVIDED

- Test device
- Specimen collection tube with extraction buffer
- Specimen collection swab for solid fecal specimens
- Specimen collection dropper for liquid fecal specimens
- Patient identification label

SIMPLE PROCEDURE

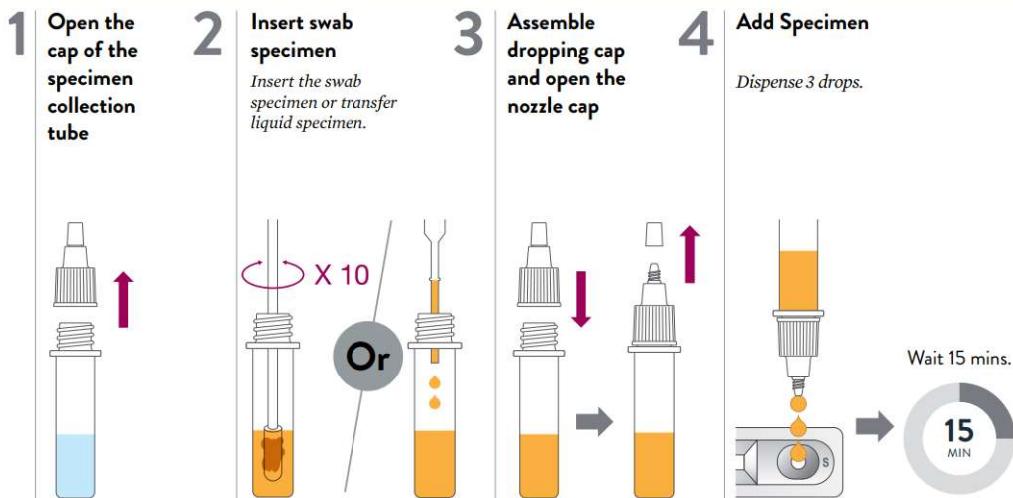

RESULTS INTERPRETATION

	Negative
	Cholera O1 Ag Positive
	Cholera O139 Ag Positive
	Cholera O1 /O139 Ag Positive
	Invalid
	C O1/O139

The presence of any test line, no matter how faint, the result is considered positive.

ORDERING INFORMATION

PRODUCT	CAT. NO.	TYPE	SPECIMEN	PACK SIZE
Cholera Ag O1/O139	44FK30	Device	Fecal	20T/Kit